

Dedicated to Delivery
Nasco
Life/form®

3 Life/form.
Year
Warranty
Simulators
& Trainers

**Child *CRiSis*™ Injectable
Training Arm
LF03612U
Instruction Manual**



Warning: This product contains dry, natural rubber.

Life/form® Products by Nasco

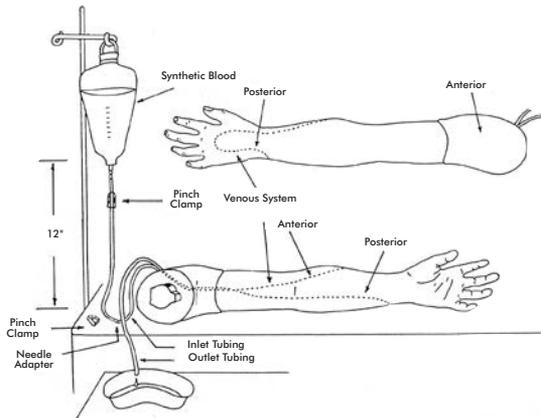


Figure 1

About the Simulator

The **Life/form**® Child Injectable Training Arm duplicates the human condition as closely as modern plastics technology allows – it is almost the real thing. Its care and treatment should be the same as with a patient; abuse or rough handling will damage the simulator – just as it would cause pain to a patient.

Although this arm will provide you long trouble-free usage, the skin and veins can be readily replaced when needed. The outer skin is easily peeled off, revealing the “core” and veins, providing, literally, a brand new arm. The life of the replaceable skin and veins will be prolonged by utilizing smaller needle sizes (22-gauge or smaller). However, if instruction with larger needle sizes is required, this can be done; the skin and veins will merely need replacing sooner. The Skin and Vein Kit is available through Nasco (see list of supplies).

List of Components

- 3 cc Syringe with Needle
- 12 cc Syringe with Needle
- 2 IV Bags
- Needle (Butterfly)
- 3 Pinch Clamps
- Small Towel
- Arm
- Case
- Mixing bottle with blood mix

Internal Structure (See figure 1.)

Internally, the vascular structure (rubber tubing) begins at the shoulder and continues under the arm, crosses the antecubital fossa forearm, makes a loop in the back of the hand, and then returns to the underarm. This venous system is constructed of special self-sealing plastic tubing, with the lumen being the approximate size of a human vein. This vascular structure has inlet tubing and outlet tubing at the shoulder, and it is via these tubes that synthetic blood is injected and removed. Thus, the techniques of blood drawing and starting intravenous infusions may be practiced on the Injectable Training Arm.

General Instructions for Use

The Injectable Training Arm comes with all of the supplies necessary to perform most procedures.

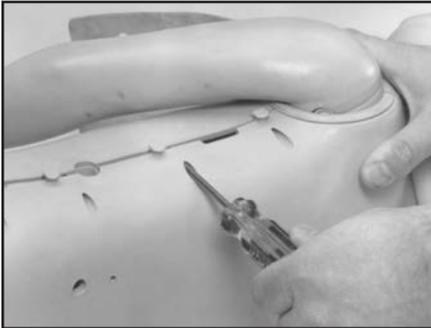


Figure 2

A. Attaching the Arm to Your Resusci® Junior* Manikin

1. Remove the existing arm by removing the six screws in the body on both sides of the shoulder. **(See figure 2.)**

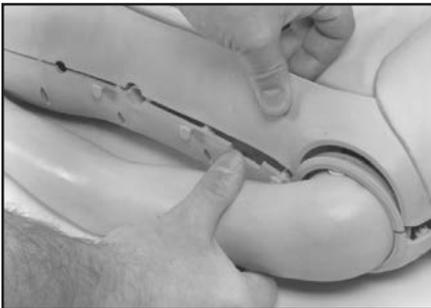


Figure 3

2. Spread the body halves at this point and pull the arm and retaining ring out. **(See figure 3.)**
3. Pull the retaining ring apart and remove it from the arm.
4. Reassemble the retaining ring through the hole in the shoulder assembly of the Child Injectable Training Arm. **(See figure 4.)**
5. Reinsert the arm into the body and replace the six screws.

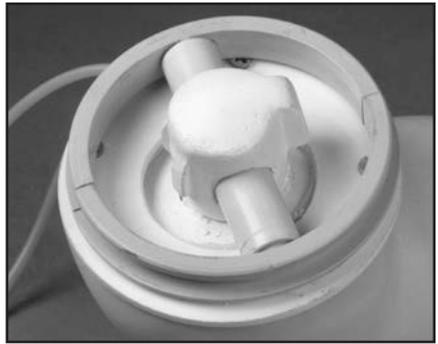


Figure 4

Note: If this arm is a replacement for the **Lifeform®** Child **CRiSis™** Manikin, simply remove the old arm by rotating it above the head and pulling out at the shoulder. Install the new arm by reversing this procedure.

B. Preparing and Drawing “Blood” from the Arm

1. Fill pint bottle containing synthetic blood concentrate with distilled water.
2. Pour the synthetic blood into one of the bags.
3. Be sure clamp on the IV tubing is closed, and hang the bag no more than 18" above the level of the arm.
4. Attach the end of the IV tubing to one of the shoulder tubings.
5. With the other shoulder tubing in a basin or sink, gradually “flush” the vascular system with synthetic blood by slowly opening the clamp. Allow some “blood” to pass through the system until the air bubbles have been eliminated.
6. Once the system is filled, use the extra pinch clamp to close off the “blood” outlet tubing. The venous system is now full of “blood” and pressurized. Be sure to leave the clamp on the IV tubing opened.

*RESUSCI® JUNIOR IS A TRADEMARK OF LAERDAL MEDICAL CORPORATION.

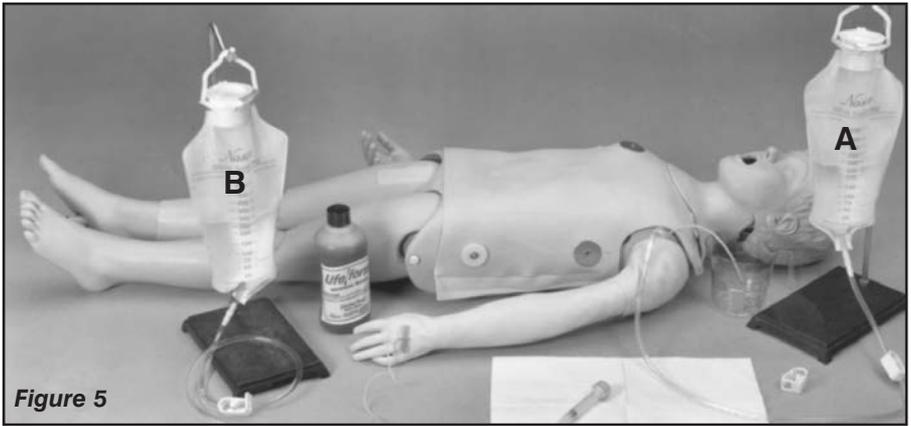


Figure 5

7. After filling the venous system according to instructions, the arm is now ready to practice drawing “blood.” “Blood” can be drawn anywhere along the pathway of the vein. (**See figure 1.**) **Distilled water** should be used to prepare the sites. Synthetic blood will actually be aspirated once the vein is properly punctured.
8. Small diameter needles (22-gauge or smaller) should be used.

C. Preparing the Arm for Intravenous Infusions

1. Close the clamps at the end of both IV bag tubes, fill with water (distilled water is recommended), and hang not more than 18" above the arm. (**See figure 5.**)
2. Appropriate intravenous infusion needles (or butterflies) should be used. Distilled water is recommended as an infusion.
3. The self-sealing simulated veins lend themselves very well to the practice of starting IV infusions, and IVs can be started anywhere along the pathway of the simulated vein. Cleanse the sites with distilled water only.

4. Attach adapter end of Bag A IV tubing into one of the shoulder tubing ends.
5. Place the other shoulder tubing end in basin or jar, and “flush” the vascular system by opening the clamp. Allow infusion (water) to pass through the system until air bubbles are eliminated. Shut off the flow at the shoulder tubing with a pinch clamp. The venous system is now full and pressurized.
6. Insert IV needle (or butterfly) in vein. “Flashback” will indicate proper insertion.
7. Close clamp on IV set A and remove pinch clamp from shoulder tubing.
8. Attach latex needle adapter to IV needle (or butterfly) and Bag B IV tubing. (**See figure 5.**) Open the clamp on Bag B.

Proof of proper procedure will then be evidenced by the flow of infusion fluid from IV bag B. Control flow rate with the clamp on IV set B. This fluid can be used over. If a more realistic experience is desired with “blood flashback” instead of water when inserting butterfly into lumen of vein, use next procedure D.

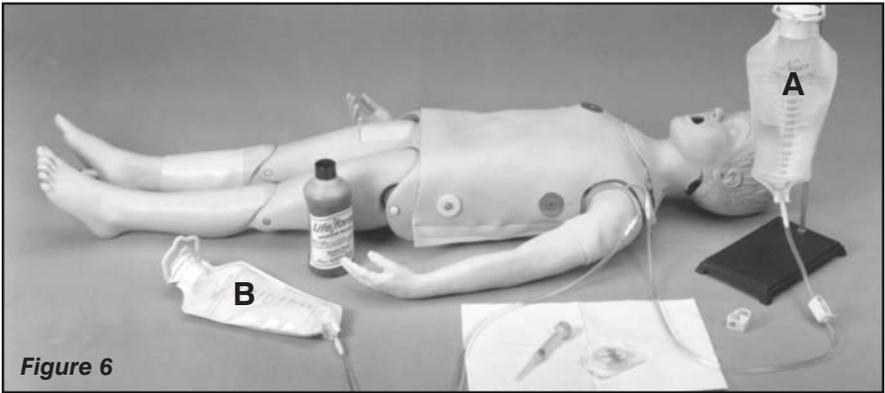


Figure 6

D. Recommended Procedure for Simultaneous IV Infusions and Drawing “Blood”

Use two IV Bag Kits. Hook up and install as shown with IV bag A and IV bag B. **(See figure 6.)**

1. Begin with synthetic blood in IV bag A. Open the clamp on both A and B to pressurize the system. “Flush” system by allowing “blood” to flow into container B until bubbles in tubing disappear, then regulate “blood” flow from bag A (using the clamp). System is now full of “blood” and pressurized. “Blood” can now be drawn anywhere along the pathway of the vein.
2. Intravenous infusion — Insert the butterfly needle into the lumen of the vein: A flashback of “blood” is proof the needle was inserted correctly. Close the clamp on the bag A tubing and disconnect it at the shoulder. Use the extra pinch clamp supplied to clamp off loose shoulder tubing. Connect the IV tubing from bag A to the butterfly needle using the special connector supplied. Open the clamp on the bag A tubing and adjust it as desired. If bag B fills, to keep the process going, simply switch

the positions of bags A and B and their IV lines **Note:** Always regulate the flow of “blood” from the bag on the stand, and be sure the clamp on the other bag is open.

Causes for Failure in Function

- A. Forgetting to open a clamp.
- B. Kinks in tubing of IV sets.
- C. Tubing pinched shut by constant pressure of clamps. Lumen remains pinched occasionally even if clamp is loosened. Slide clamp to new position and, with fingers, manipulate tubing at pinched site to restore lumen. In heavy use, slide clamp to new position on tubing from time to time to prevent the “permanent pinch” caused by constant clamp pressure. Replace IV kit.
- D. If these measures do not unclog the venous system, try using a large (50 cc) syringe to force fluid through the tubing.
- E. If none of these measures work, peel back the skin (soap up arm and skin generously with Ivory® liquid detergent) of the arm to the knuckles (do not remove from fingers), and examine all tubing for possible kinks. Soap up arm and skin generously with Ivory® liquid detergent, and return skin over arm.

Care of Simulator

After each class use, disconnect “blood” and flush the venous system. Return synthetic blood to the storage bottle. Remove pinch clamps and IV sets from arm. Use tap water to flush venous system and wash outside of arm with Ivory® liquid detergent and water. Excess water may be removed from the arm by raising the hand, lowering the shoulder, and draining it into a sink or basin. Always remove the pinch clamp from shoulder tubing and drain excess water from veins before storing.

Ordinary stains can be removed by washing with soap and warm water. Newsprint, similar printed paper, plastic, or ball-point pen will permanently stain the simulator if prolonged contact occurs. Stubborn stains may be removed with Nasco Cleaner (LF09919U) simply by dispensing it on the area and wiping with a soft cloth or paper towel.

Cautions

1. This synthetic blood is specially formulated to be compatible with the self-sealing veins and plastics used in manufacturing the arm.
2. **DO NOT** use dull or burred needles, as these will cause leaks in the system. Burred needles will cause permanent damage. Use smaller needles (22-gauge or smaller).
3. **DO NOT** allow “blood” to dry on simulator – it may stain the arm.
4. Use only 500 cc of infusion fluid, as a larger amount will also increase the pressure of the venous system, resulting in leaks.
5. **DO NOT** clean the simulator with solvents or corrosive material, as they will damage it.

6. **DO NOT** use for subcutaneous injection. Nasco’s Intradermal Injection Simulator (LF01008U) is specially designed for intradermal injection training and practice.
7. Nasco Vein Tubing Sealant Kit (LF01099U) will extend the useful life of the tubing.

Supplies/Replacement Parts for Child Injectable Training Arm

- LF00845U **Life/form**® Venous Blood, 1 quart
- LF00846U **Life/form**® Venous Blood, 1 gallon
- LF01099U Vein Tubing Sealant Kit
- LF03629U Replacement Skin and Vein Kit
- LF09919U Nasco Cleaner

Other Available *Life/form*® Simulators

- LF00698U** Adult Injectable Arm (White)
LF00855U Male Catheterization
LF00856U Female Catheterization
LF00901U Prostate Examination
LF00906U Ostomy Care
LF00929U Surgical Bandaging
LF00957U Enema Administration
LF00958U Pediatric Injectable Arm
LF00961U Intramuscular Injection
LF00984U Breast Examination
LF00995U Arterial Puncture Arm
LF00999U Pediatric Injectable Head
LF01005U First Aid Arm
LF01008U Intradermal Injection Arm
LF01012U Heart Catheterization (TPN)
LF01019U Ear Examination
LF01027U Peritoneal Dialysis
LF01028U Suture Practice Arm
LF01034U Suture Practice Leg
LF01036U Spinal Injection
LF01037U Hemodialysis Practice Arm
LF01038U Episiotomy Suturing Set
LF01042U Suture Kit
LF01062U Pelvic, Normal & Abnormal
LF01063U Stump Bandaging, Upper
LF01064U Stump Bandaging, Lower
LF01069U Cervical Effacement
LF01070U Birthing Station
LF01082U Cricothyrotomy
LF01083U Tracheostomy Care
LF01084U Sigmoidoscopic Examination
LF01087U Central Venous Cannulation
LF01095U Blood Pressure Arm
LF01108U Infant Intraosseous Infusion
LF01121U Advanced IV Arm
LF01131U Venipuncture and Injection Arm
LF01139U Advanced IV Hand
LF01142U Auscultation Trainer
LF01143U Testicular Exam
LF01152U Male & Female Catheter
LF01155U Advanced CPR Dog
LF01162U Venatech IV Trainer
LF01174U NG Tube & Trach Skills
LF01184U Venatech IM & Sub Q
LF01193U Special Needs Baby
LF03000U **CPARLENE**® Series
LF03601U Adult Airway Management Trainer with Stand
LF03602U Adult Airway Management Manikin
LF03609U Child Airway Management Trainer with Stand
LF03616U Child **CRiSis**™ Manikin
LF03617U Deluxe Child **CRiSis**™ Manikin with Arrhythmia Tutor
LF03620U PALS Update Kit
LF03623U Infant Airway Management Trainer with Stand
LF03632U Child Intraosseous Infusion/ Femoral Access Leg on a Stand
LF03633U Child Airway Management Trainer Torso
LF03693U **Basic Buddy**® CPR Manikin
LF03699U "Airway Larry" Airway Management Trainer
LF03709U Infant **CRiSis**™ Manikin
LF03720U **Baby Buddy**™ Infant CPR Manikin
LF03750U Fat Old Fred
LF03760U Airway Management/Cricoid Pressure Trainer
LF03770U Chest Tube
LF03953U **CRiSis**™ Manikin, Complete
LF03955U Deluxe **CRiSis**™ Manikin
LF03956U Deluxe "Plus" **CRiSis**™ Manikin
LF03965U Adult **CRiSis**™ Auscultation Manikin
LF03966U Adult **CRiSis**™ Auscultation Manikin with ECG Simulator
LF04000U **GERI**™/**KERI**™ Manikin Series
LF04200U Adult Sternal Intraosseous Infusion
LF06001U CPR Prompt® Adult/Child Manikin
LF06012U CPR Prompt® Infant Manikin
LF06200U CPR Prompt® Keychain Rescue Aid
LF06204U CPR Prompt® Rescue and Practice Aid

Nasco Fort Atkinson

901 Janesville Avenue, P.O. Box 901
Fort Atkinson, Wisconsin 53538-0901
1-800-558-9595

eNasco.com • E-mail: lifeform@eNasco.com